

FIG. 1A

+

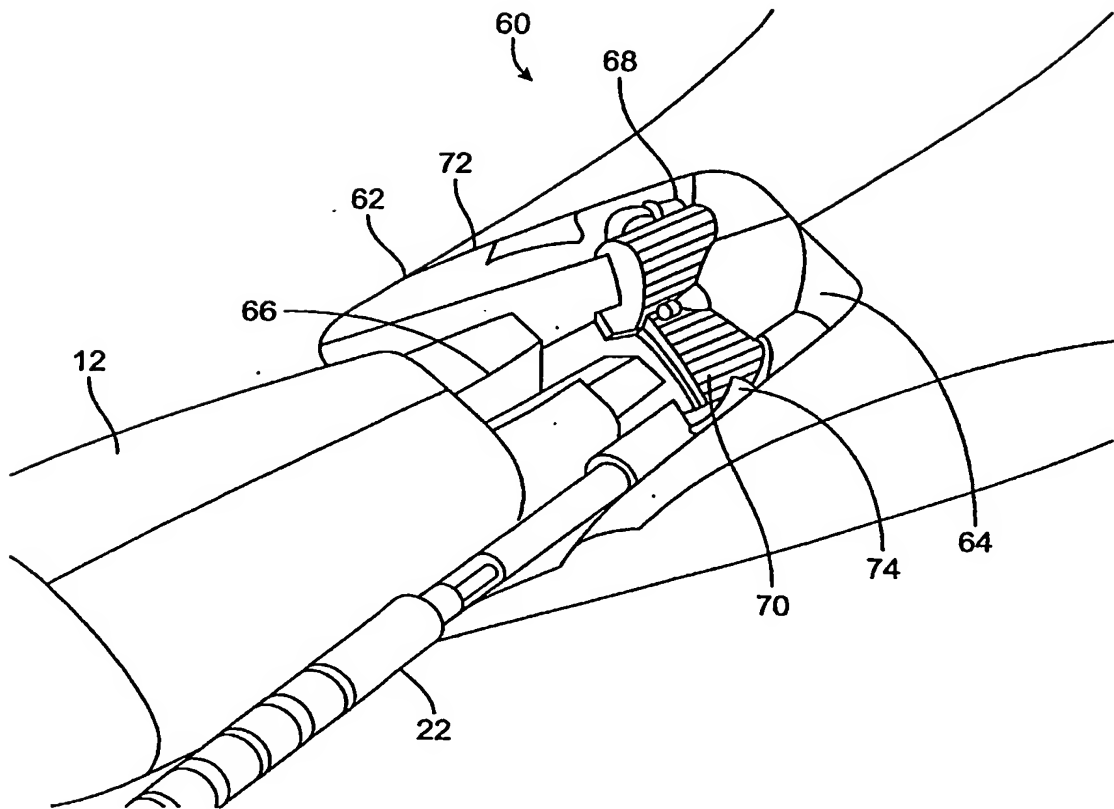


FIG. 1B

+

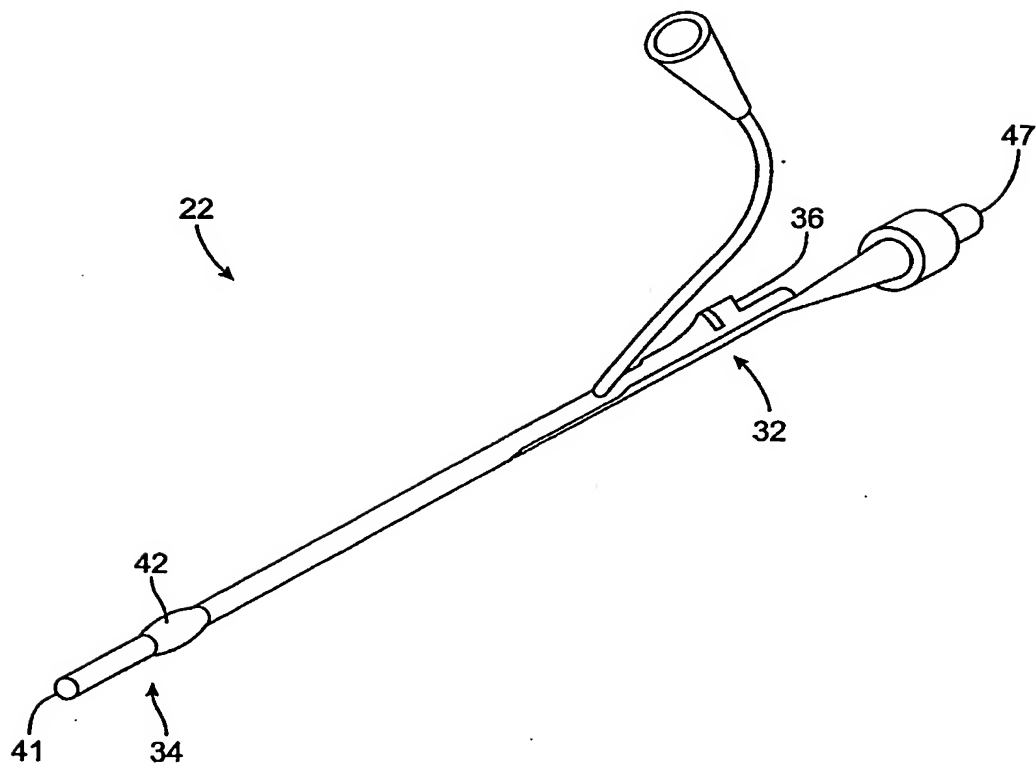


FIG. 2

+




FIG. 3

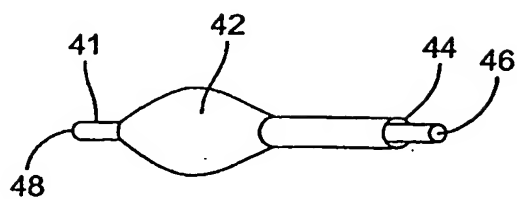


FIG. 4

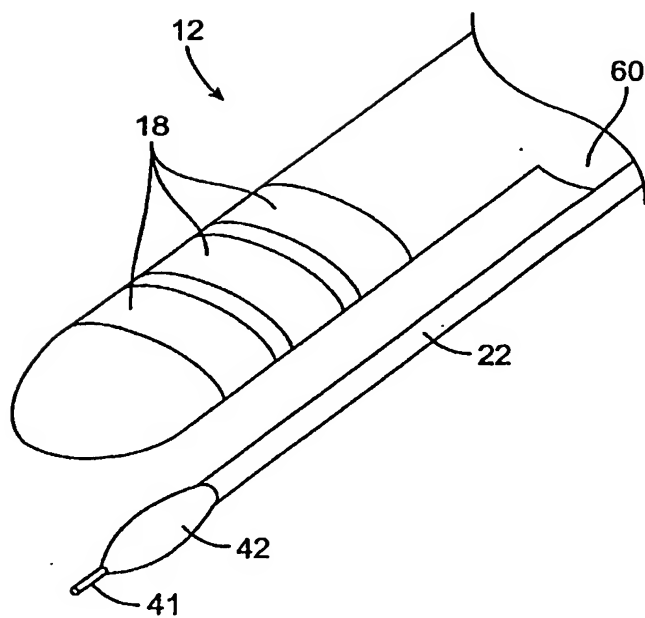


FIG. 5

+

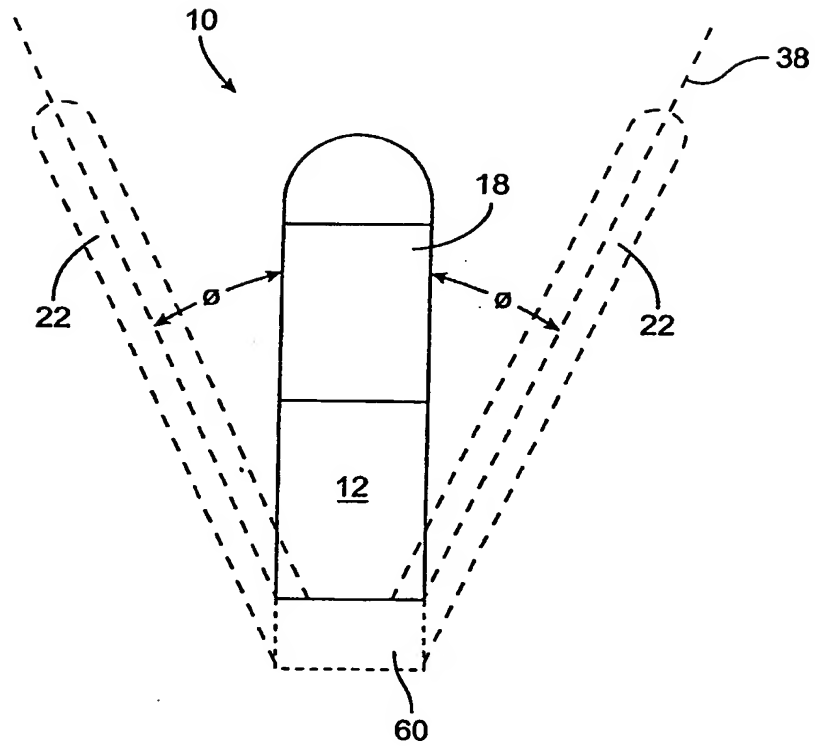


FIG. 6

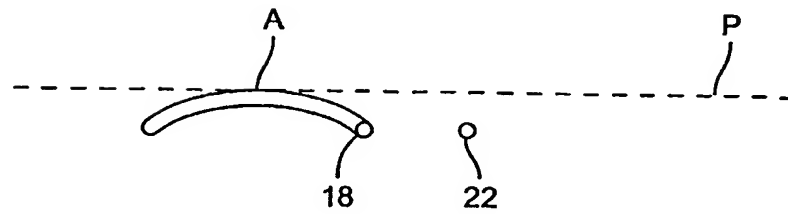


FIG. 7

+

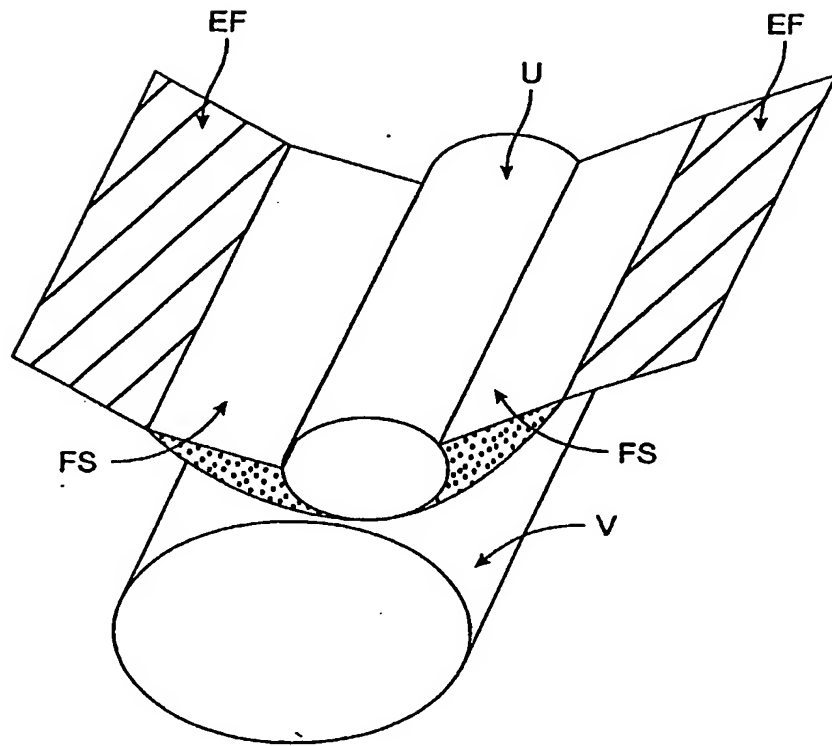


FIG. 8

+

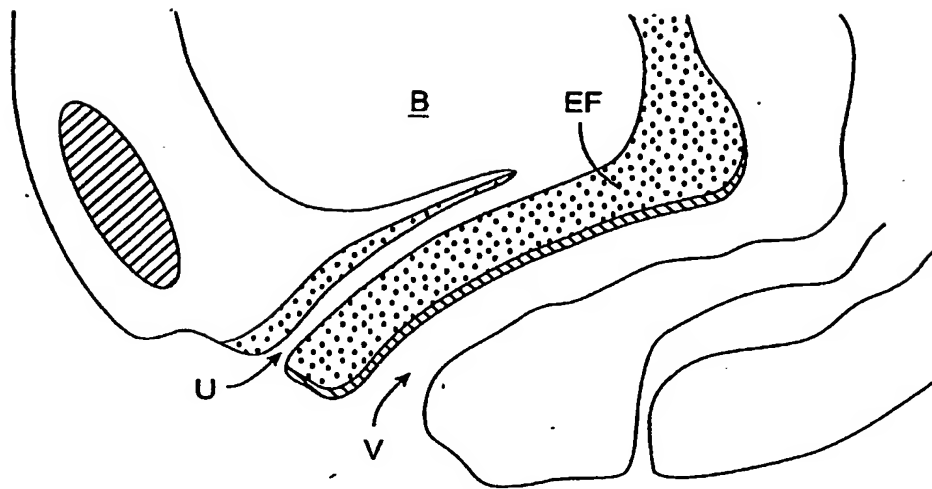


FIG. 9

FIG. 1 is a schematic diagram of a medical device 10 in a closed position. The device includes a main body 12 with a rounded top and a vertical shaft 18. A handle 22 is attached to the side of the shaft 18 via a pivot joint 86. A locking mechanism 88 is located at the pivot joint. A dashed line indicates the handle's position when the device is open.

FIG. 9B



+

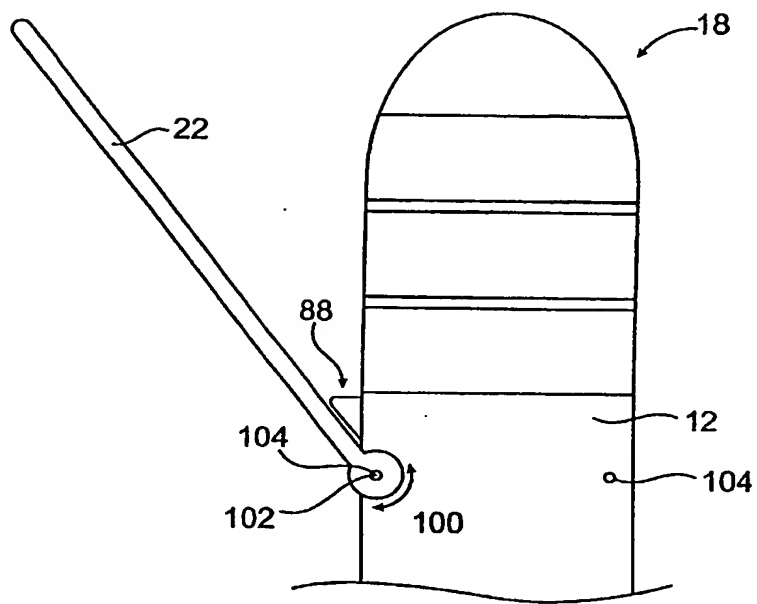


FIG. 9C

+

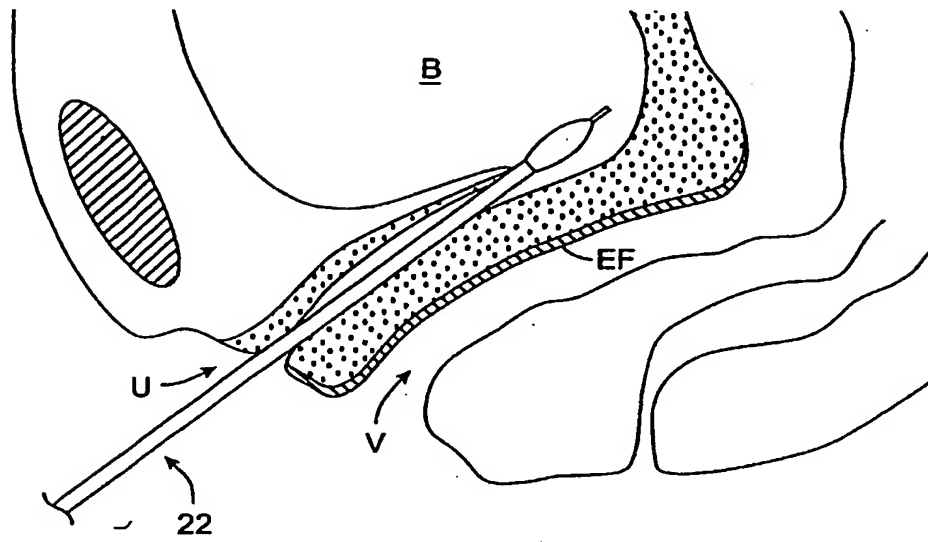


FIG. 10

+

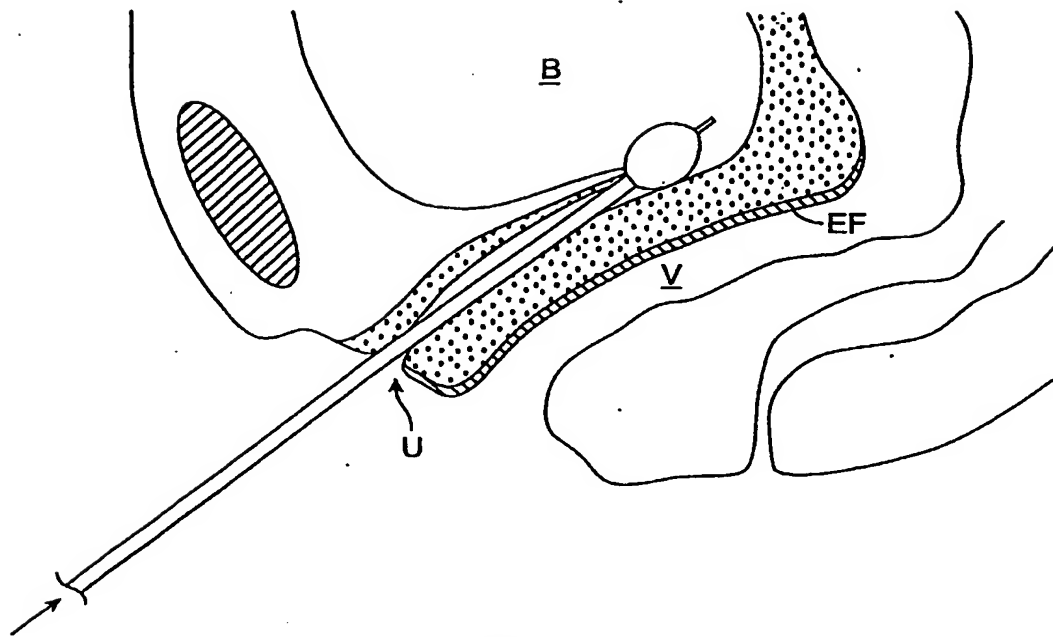


FIG. 11

+

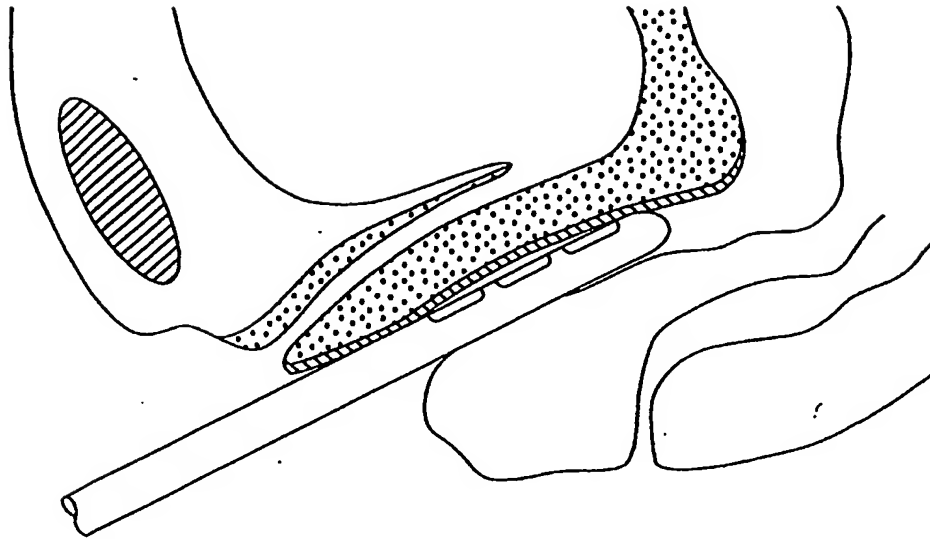


FIG. 12

+

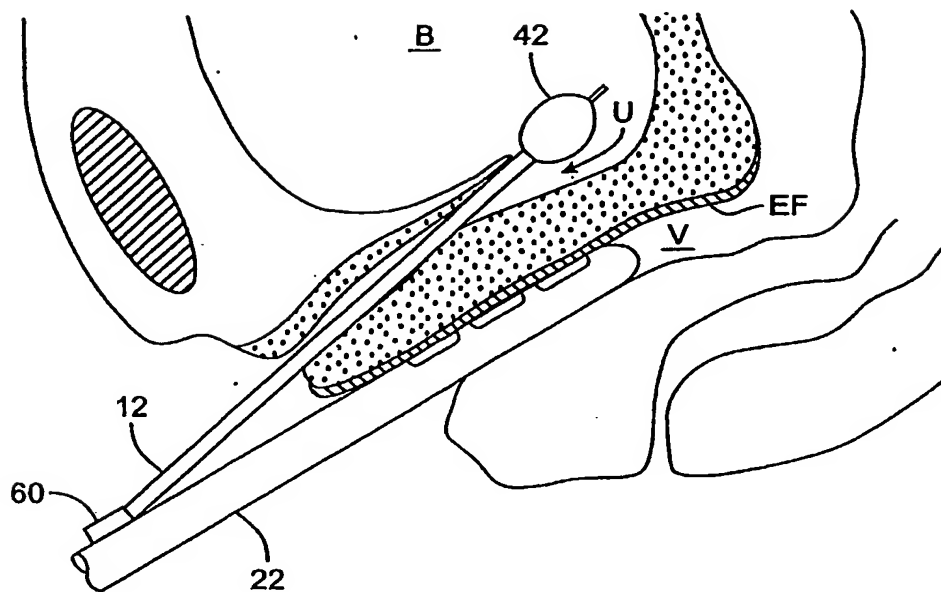


FIG. 13

+

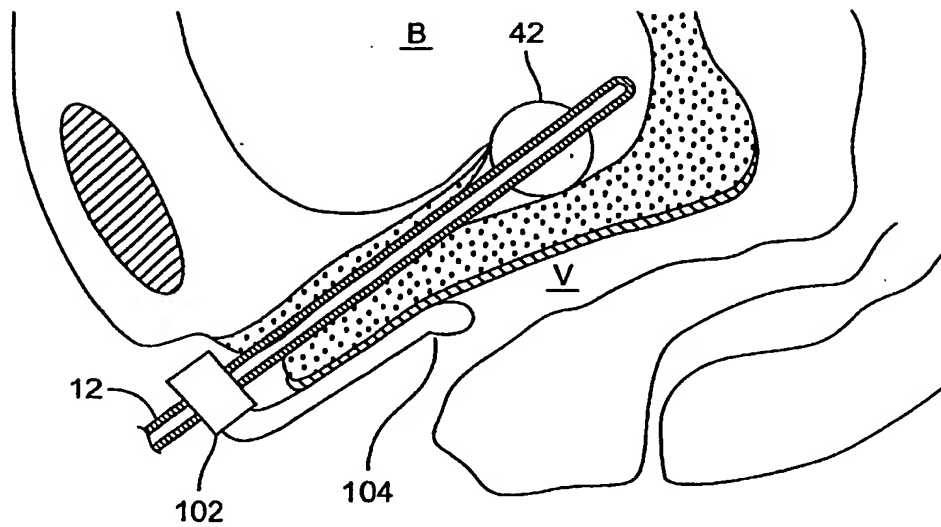


FIG. 14

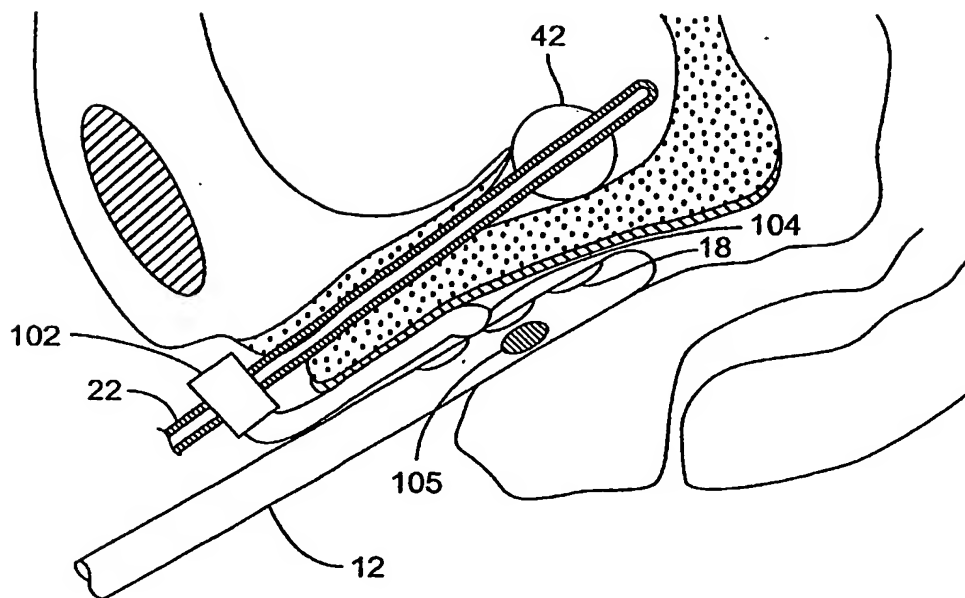


FIG. 15

+

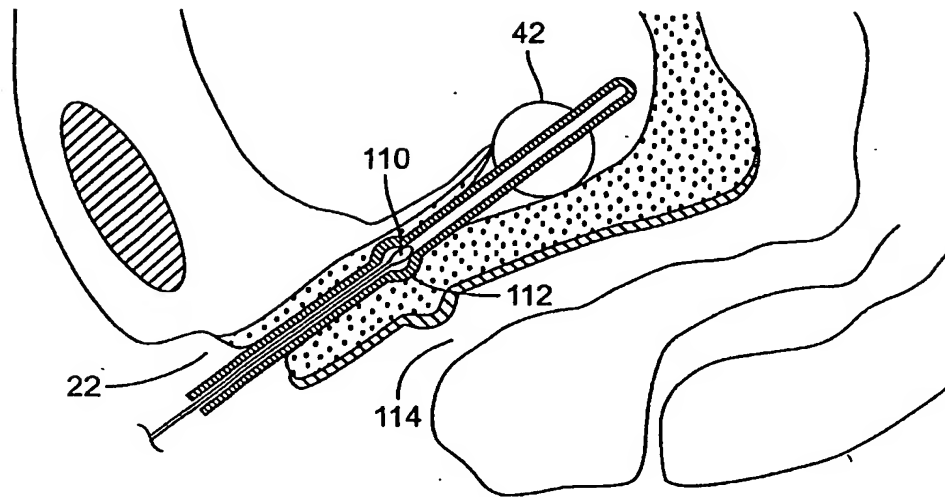


FIG. 16



+

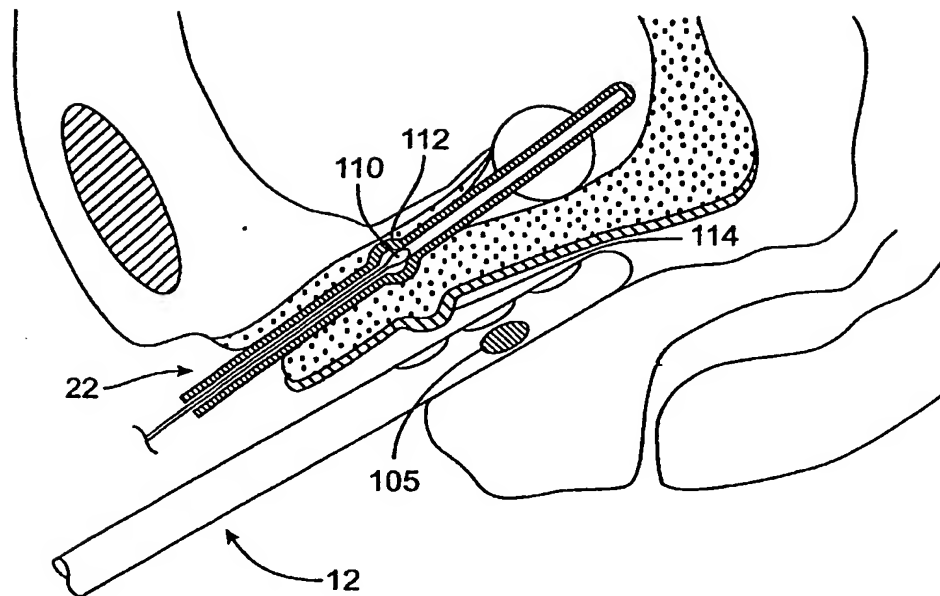


FIG. 17

+

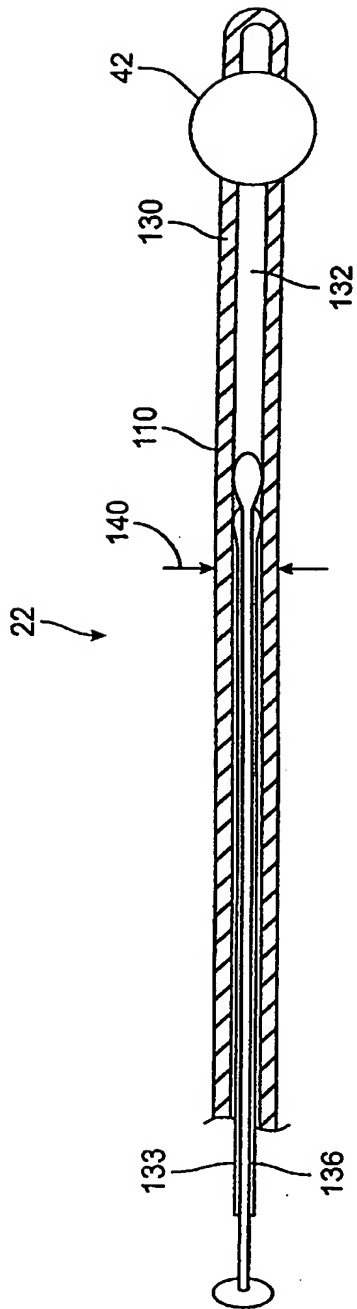


FIG. 18A

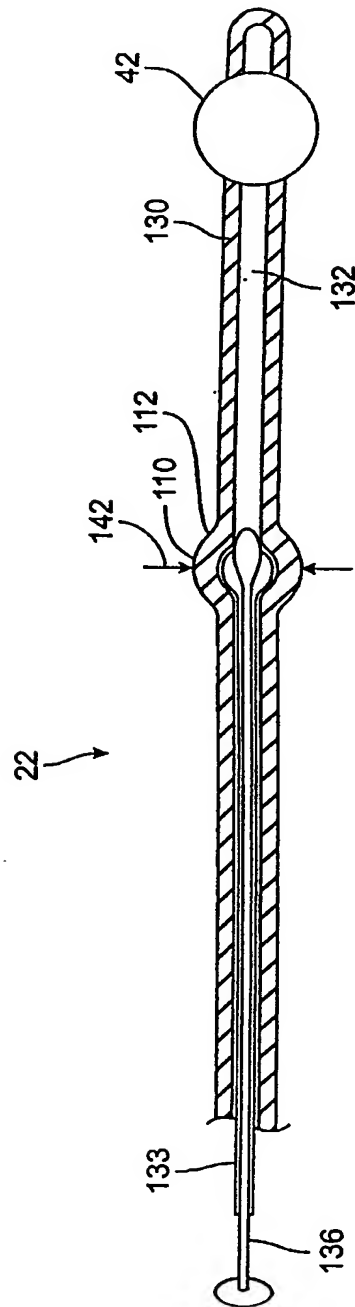


FIG. 18B

+

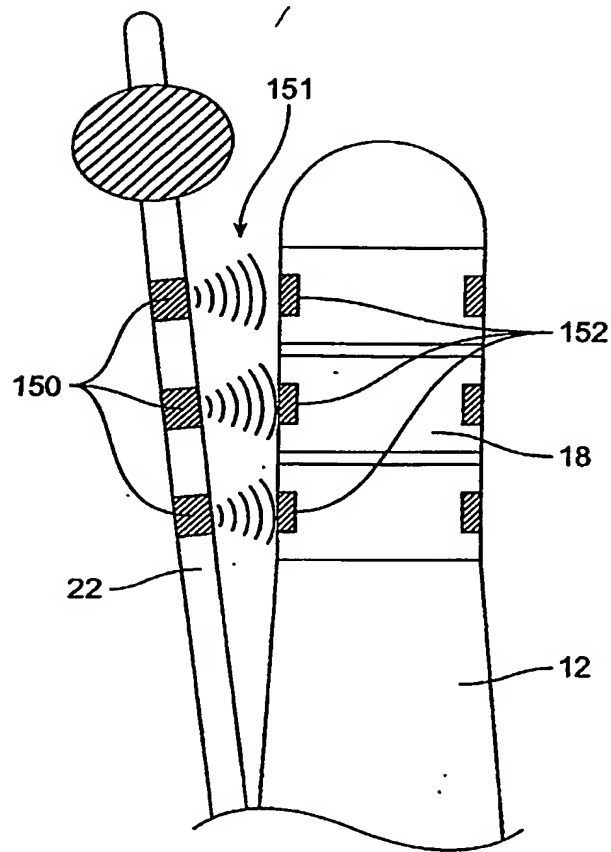


FIG. 19A

+

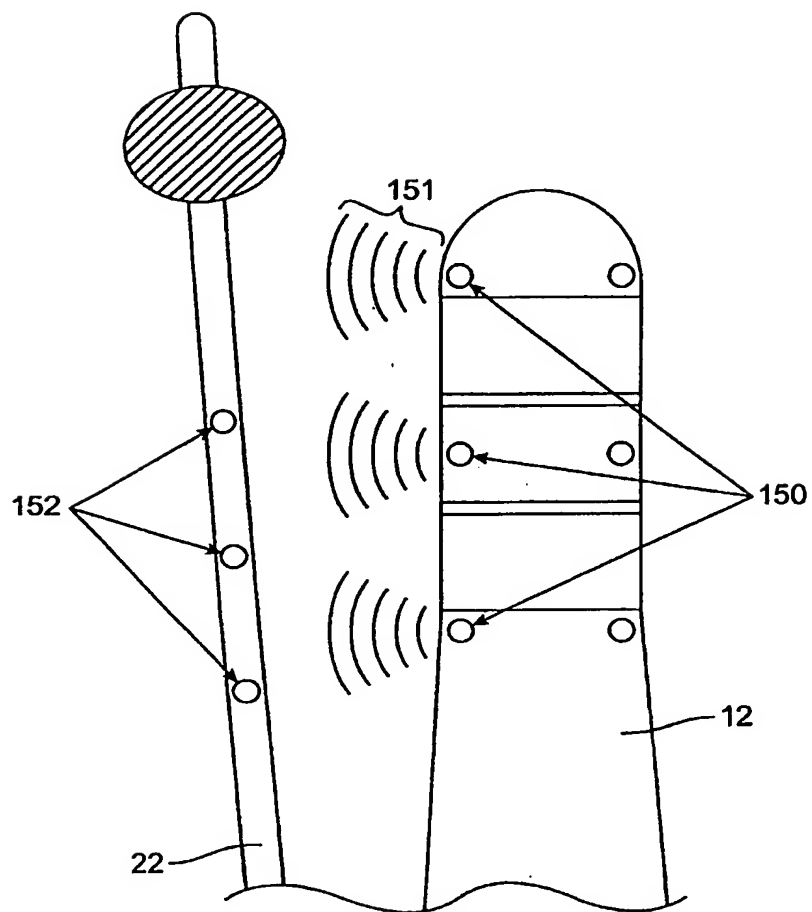


FIG. 19B

+

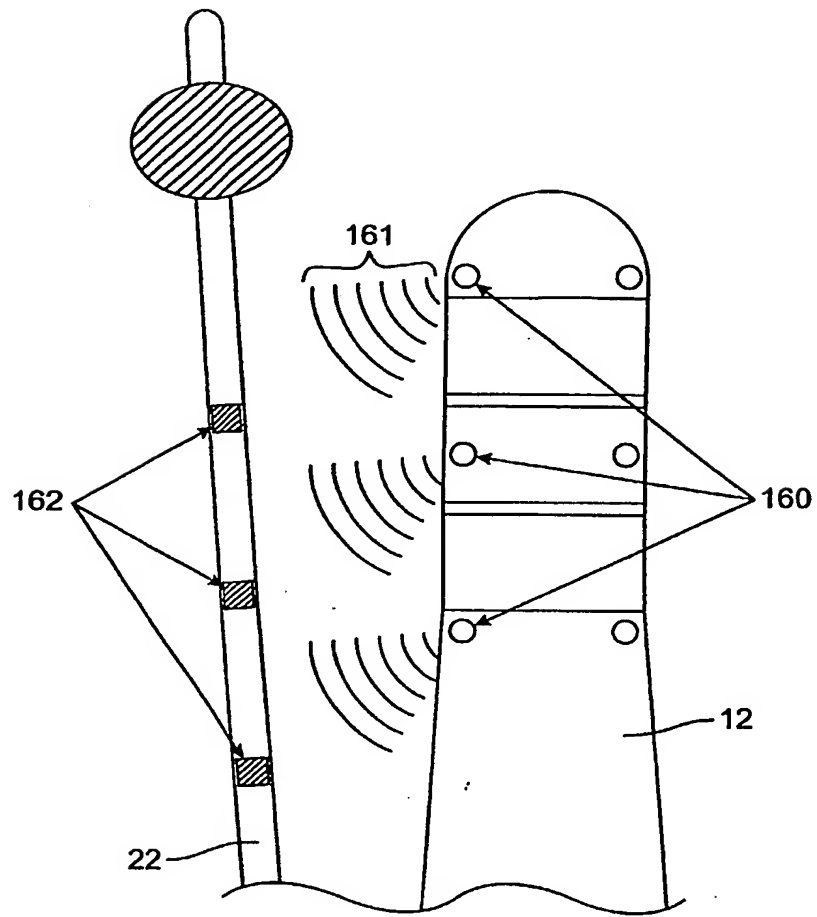


FIG. 20A

+

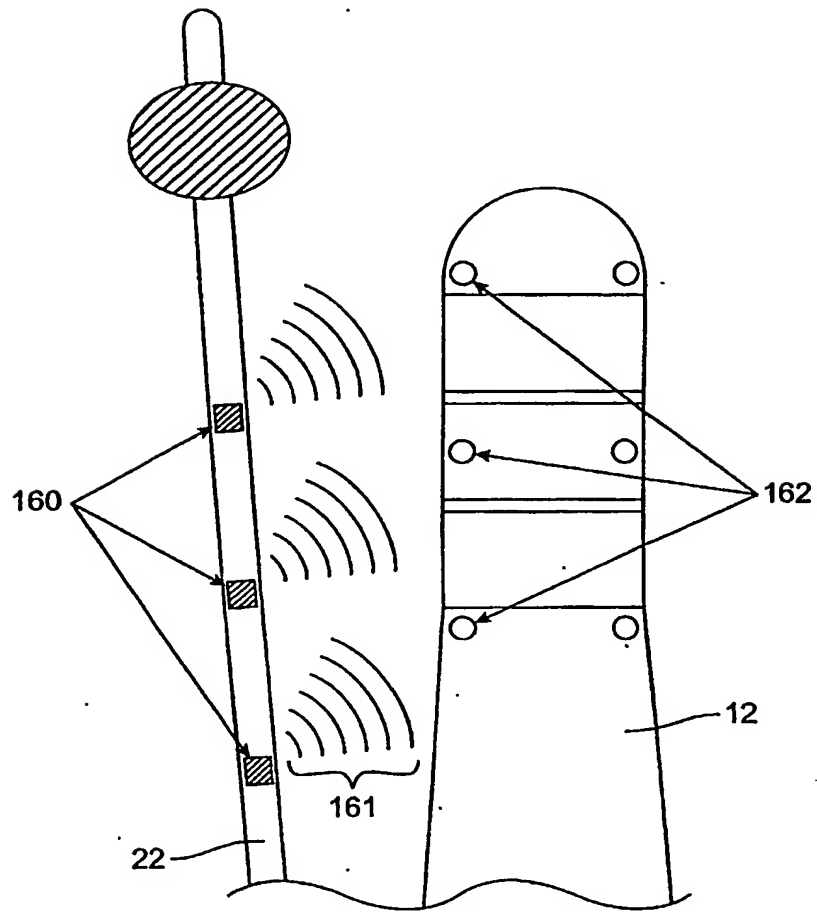


FIG. 20B

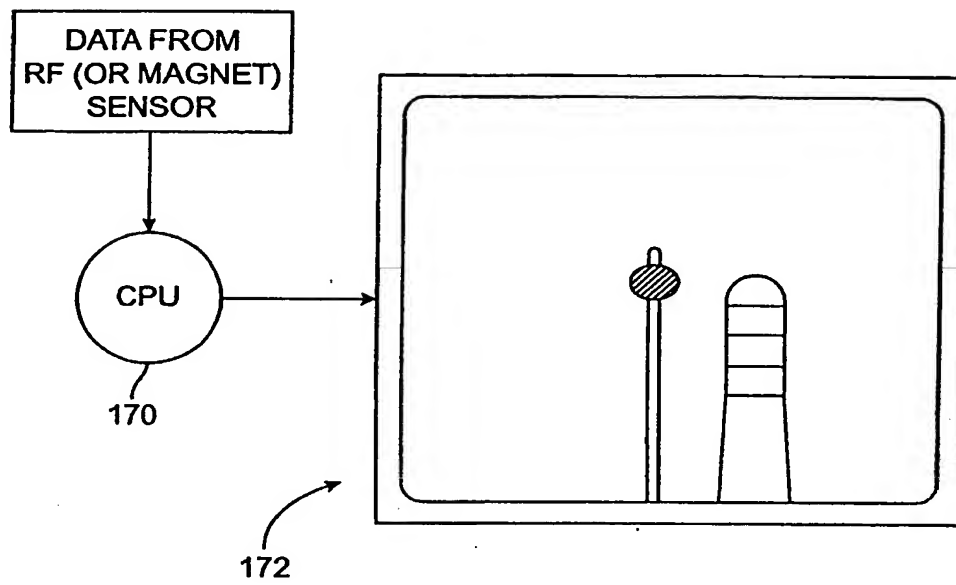


FIG. 21

+

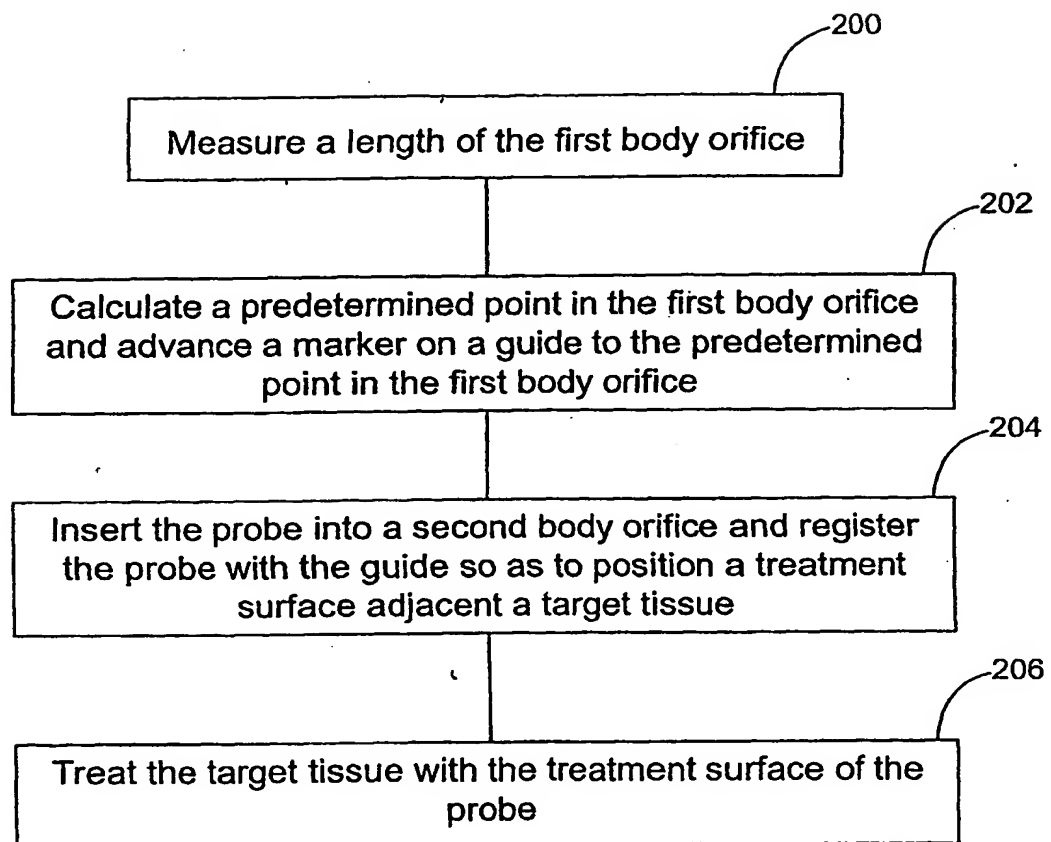


FIG. 22



+

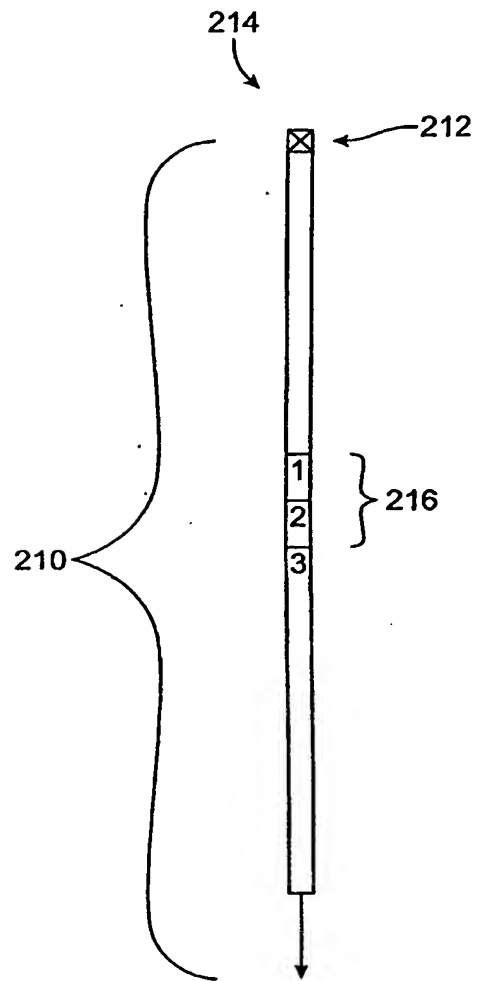


FIG. 23A

+

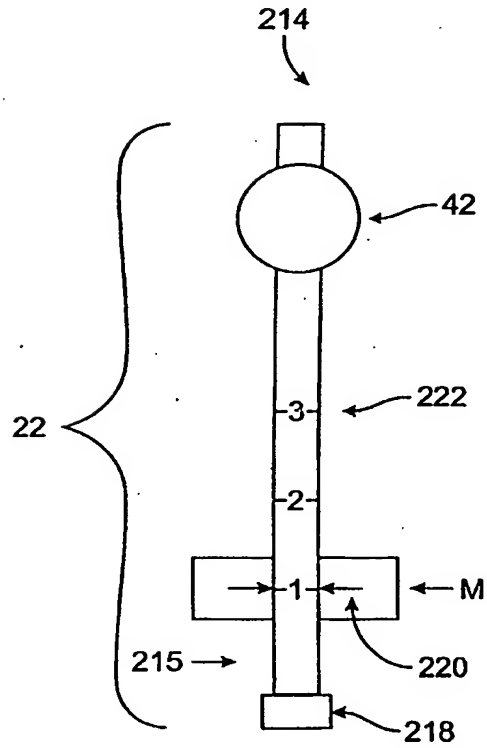


FIG. 23B

+

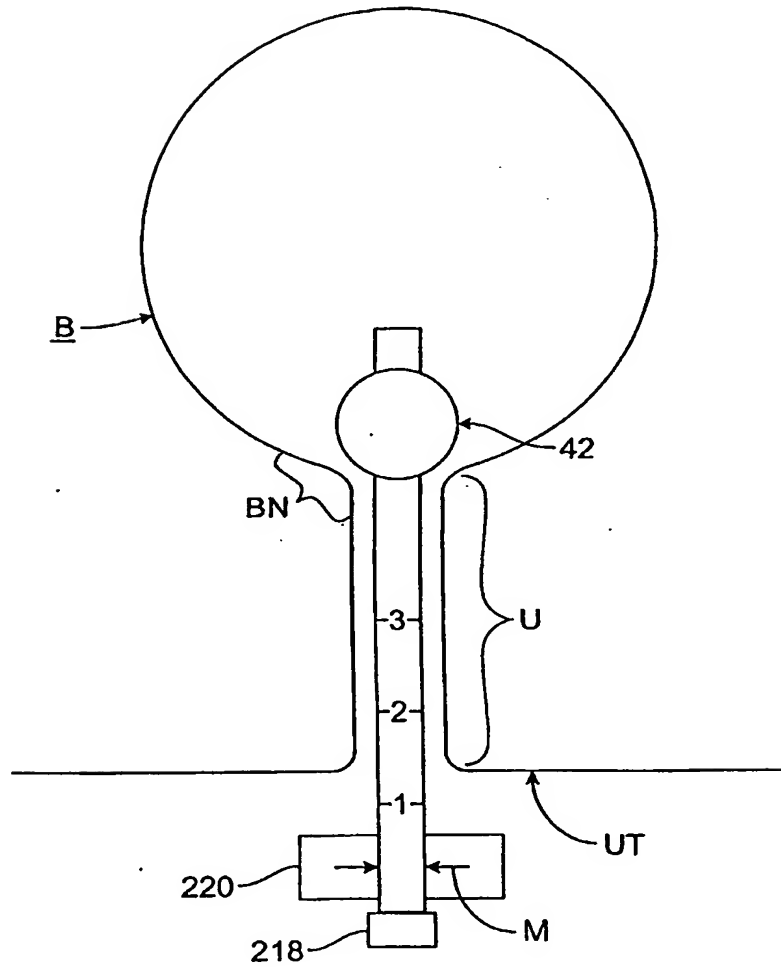


FIG. 23C

+

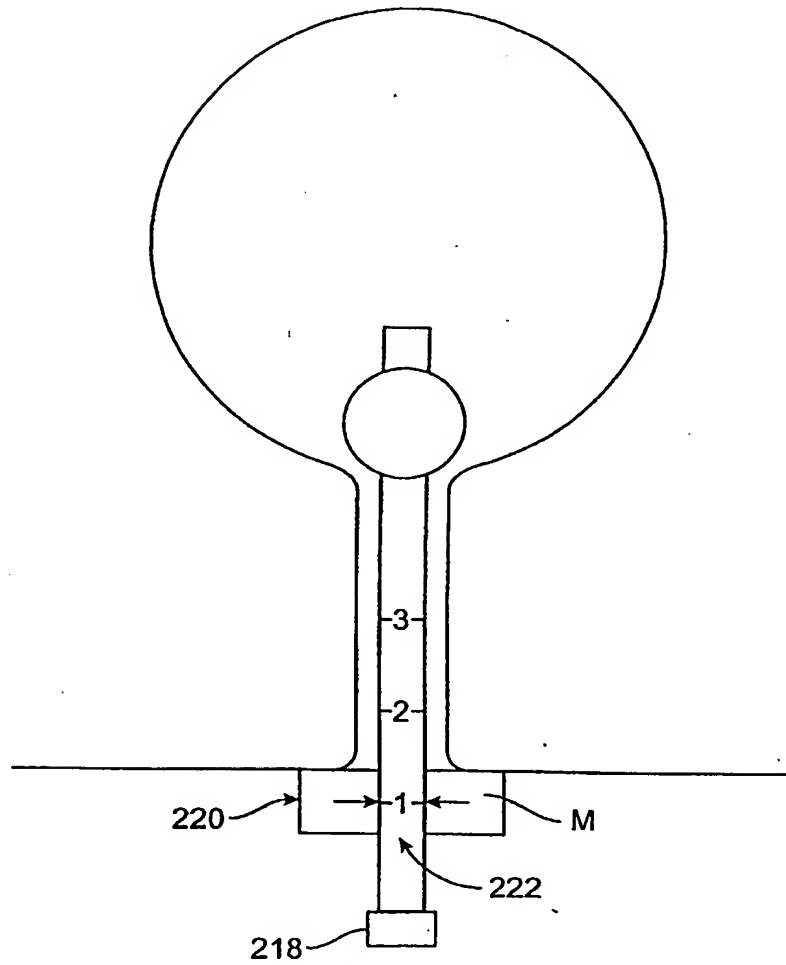


FIG. 23D

+

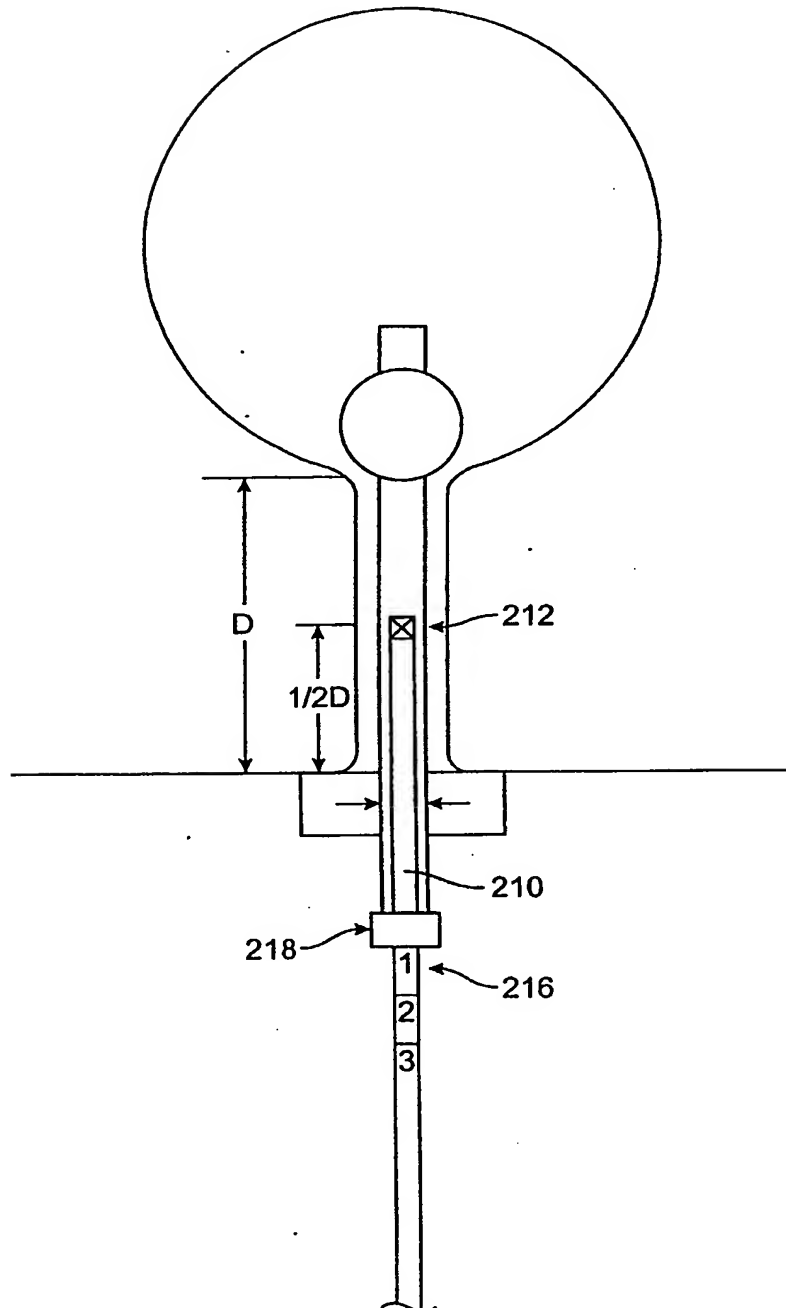


FIG. 23E

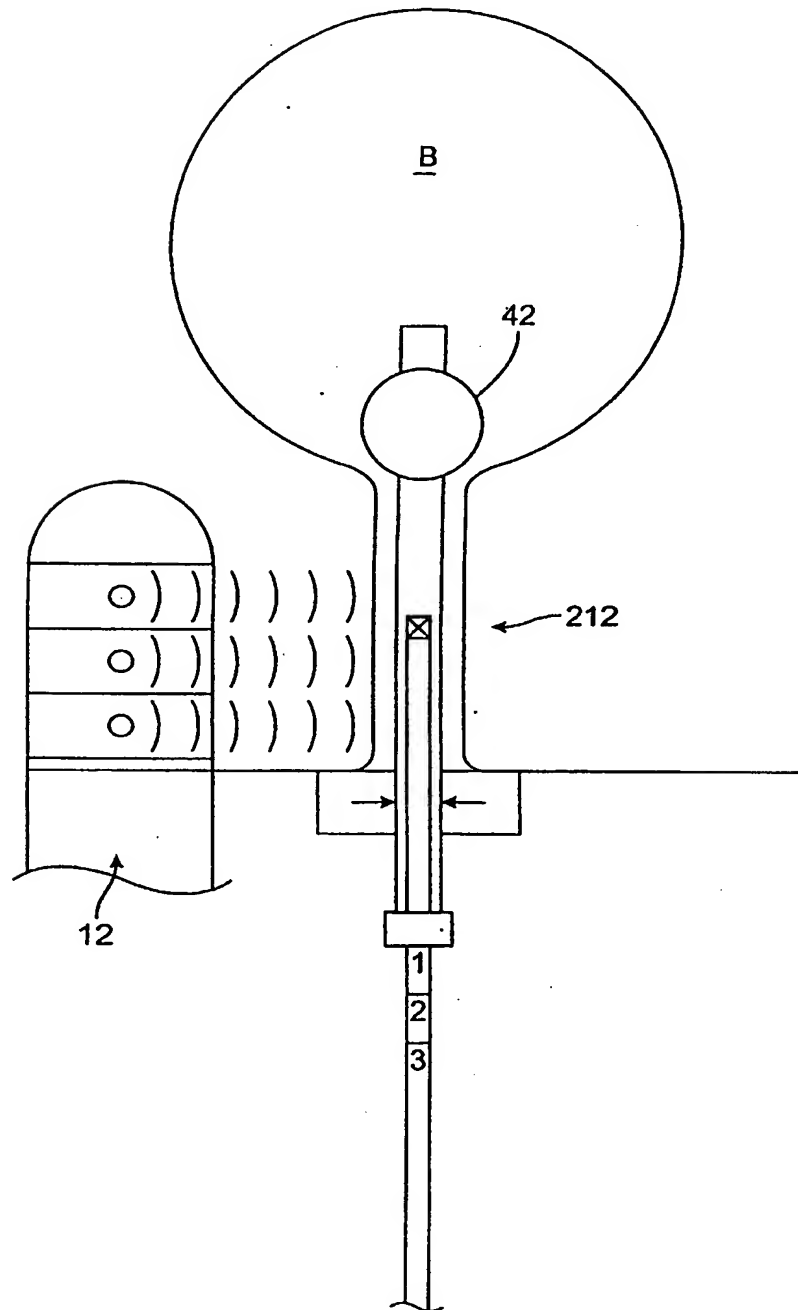


FIG. 23F

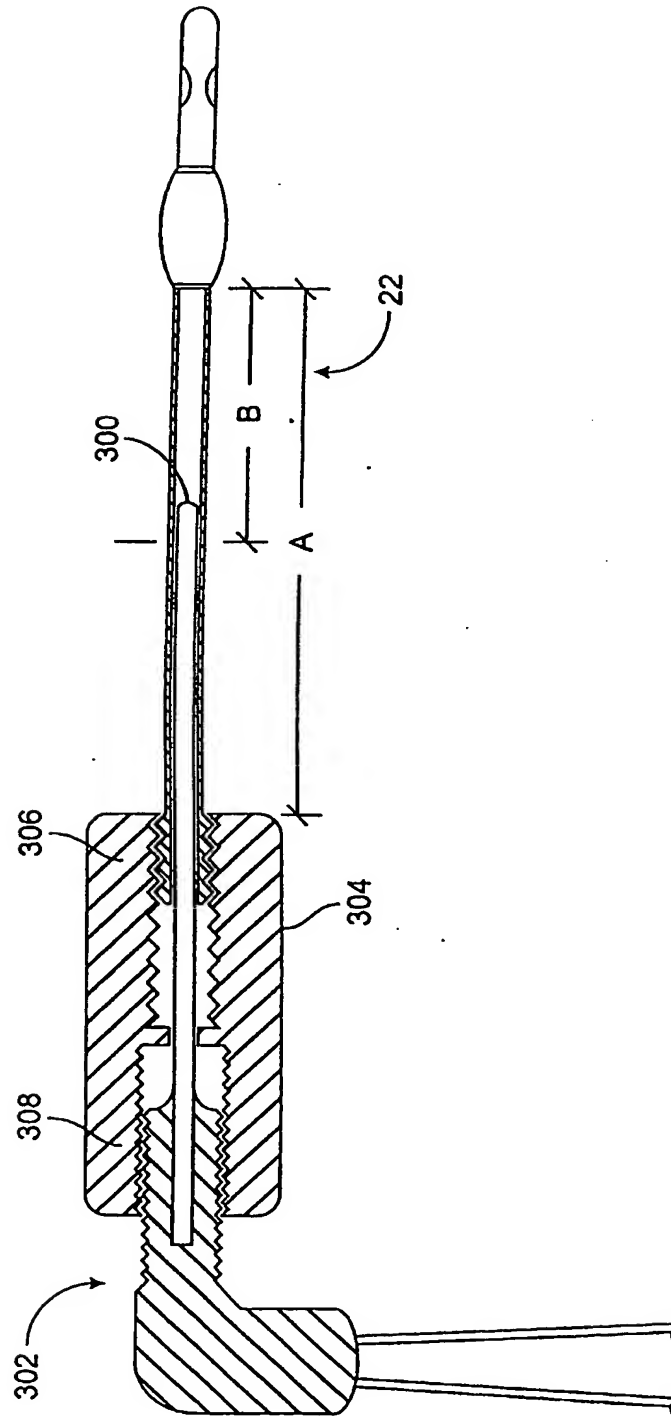


FIG. 24A

+

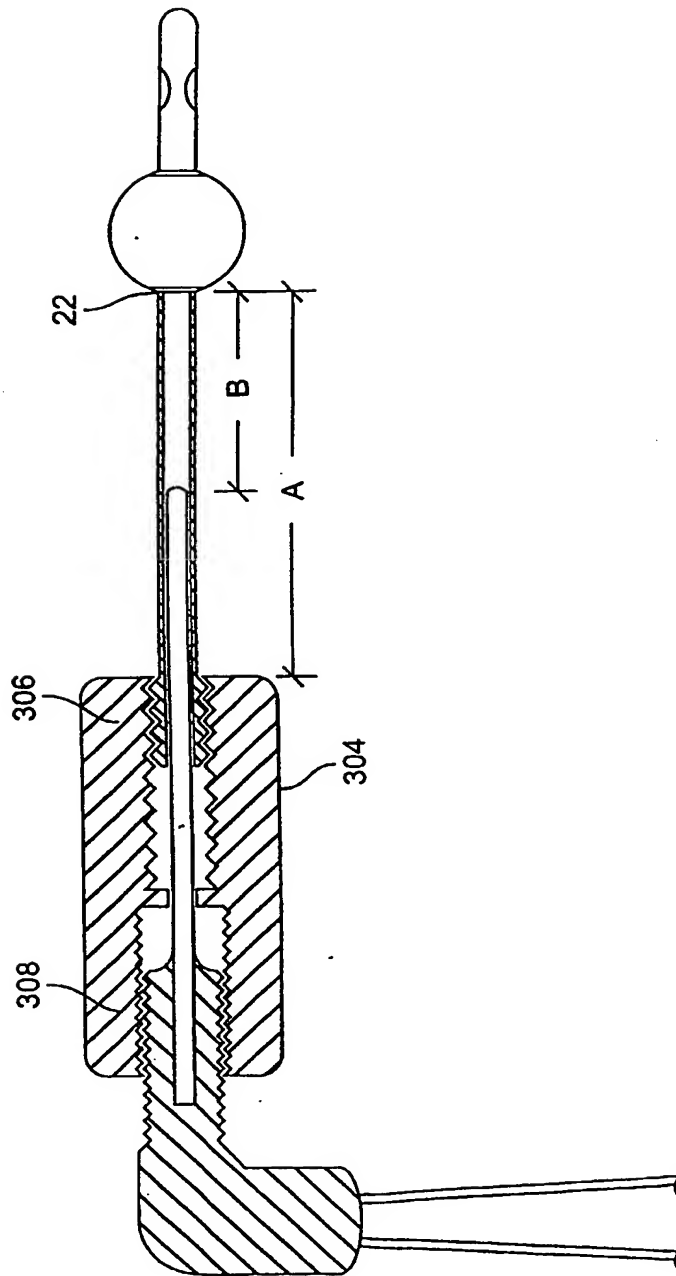


FIG. 24B



+

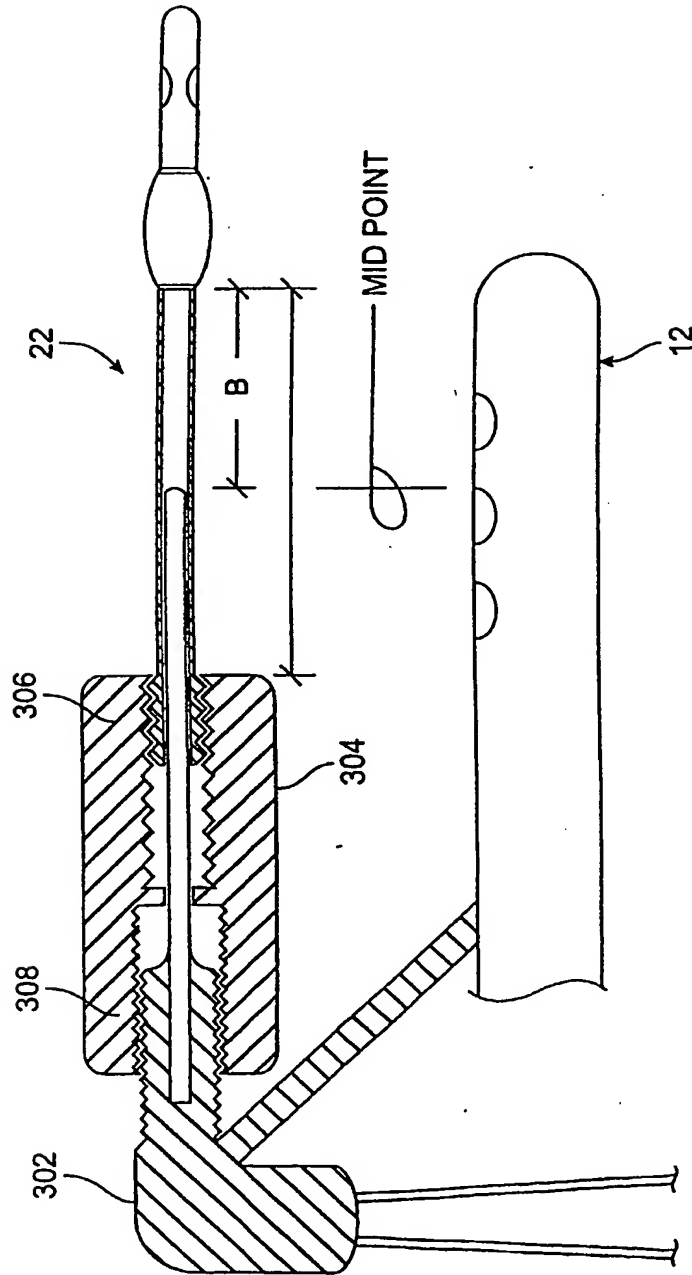


FIG. 24C

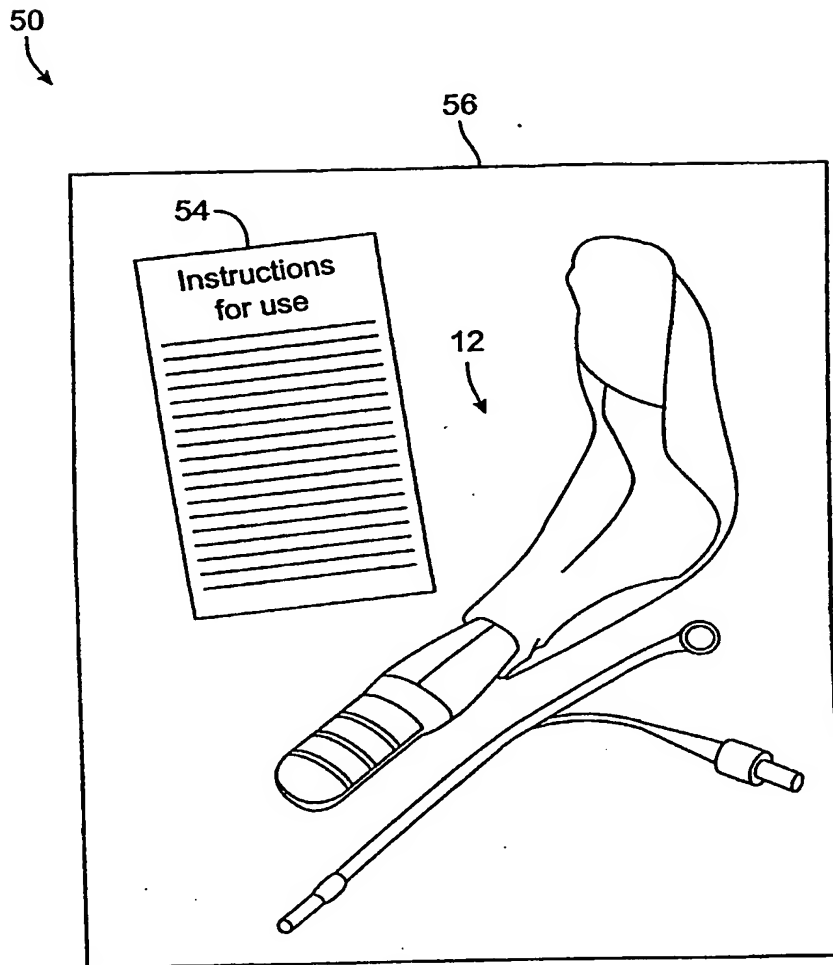


FIG. 25

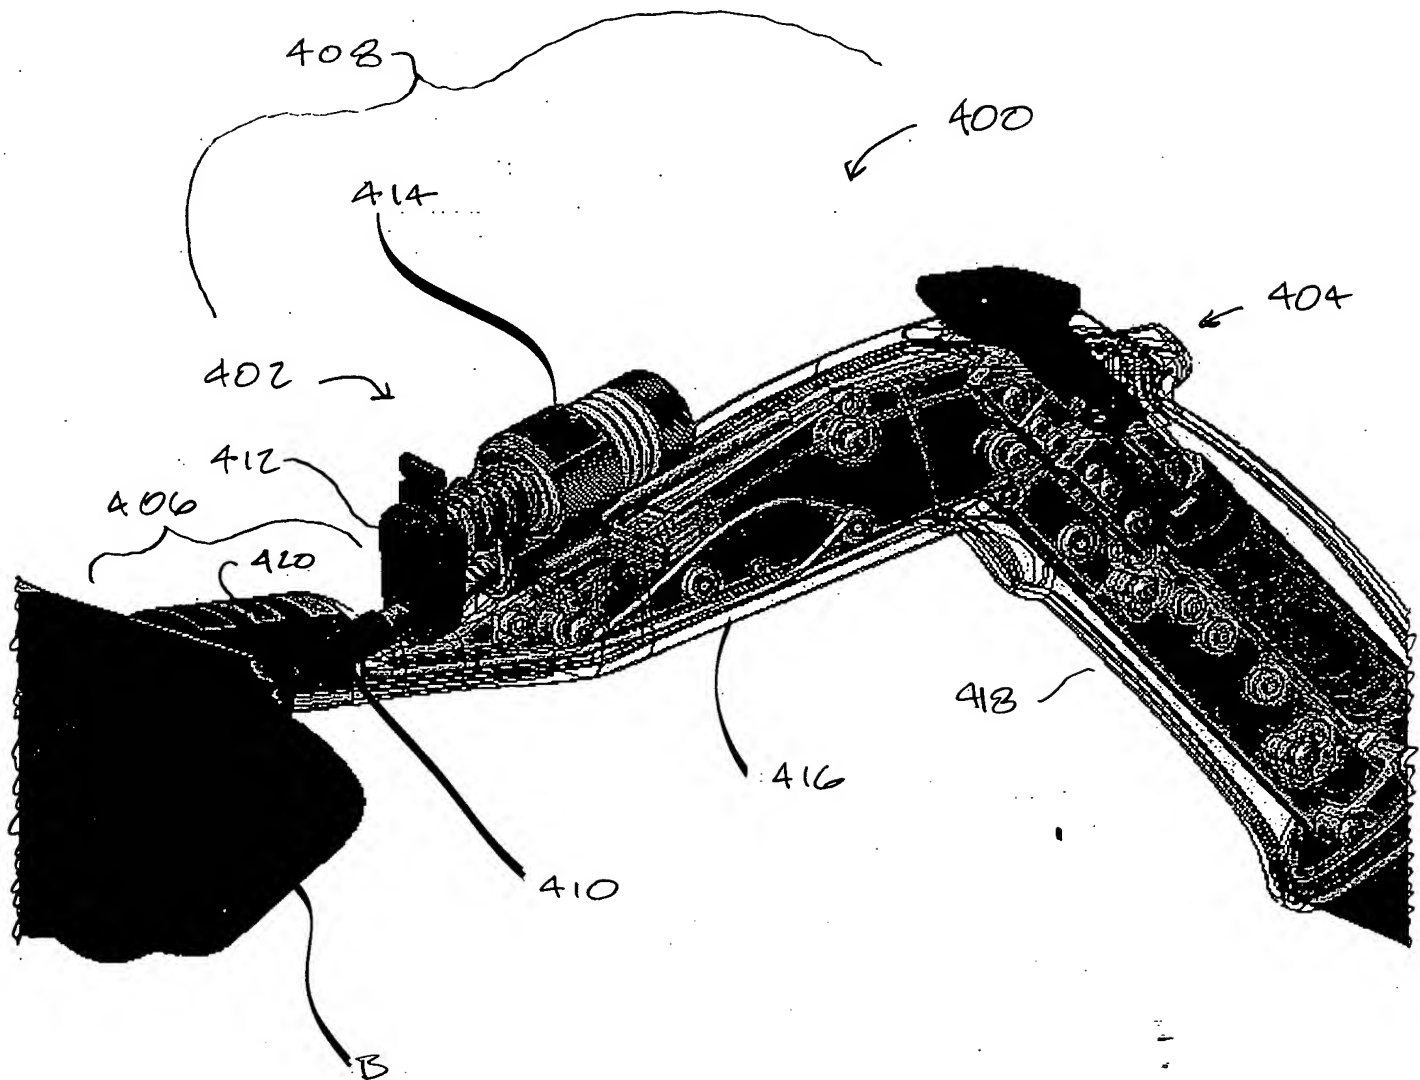


FIG - 26

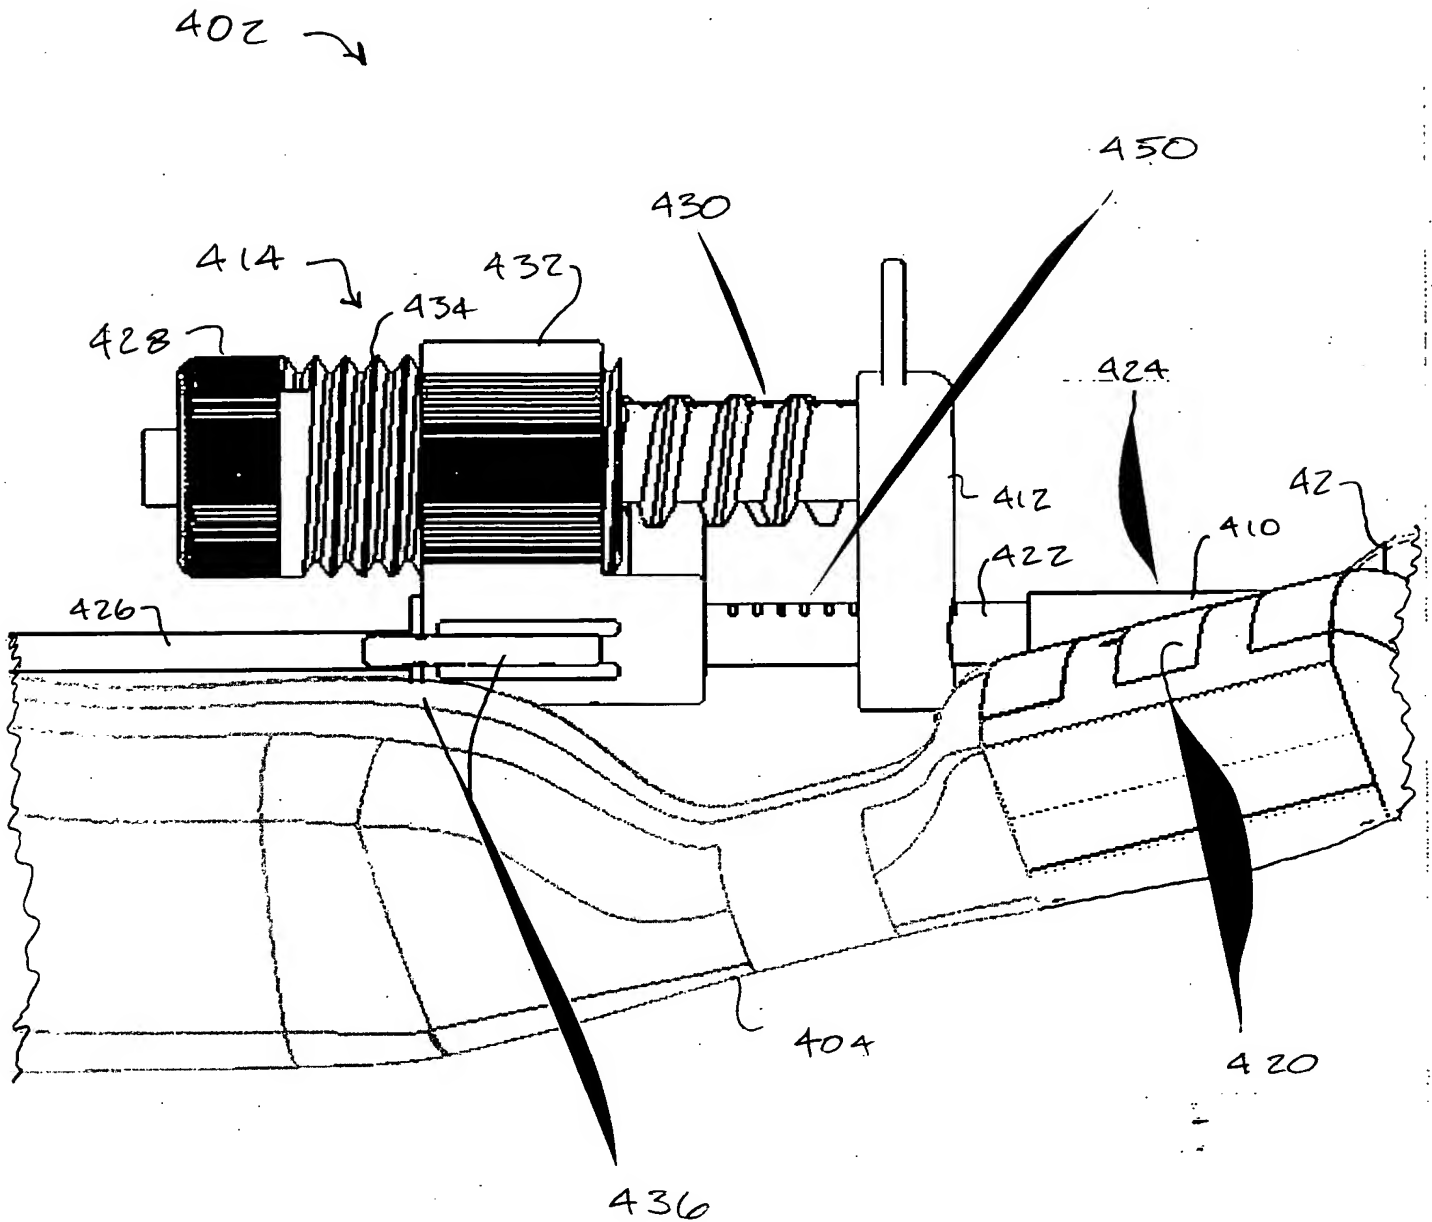
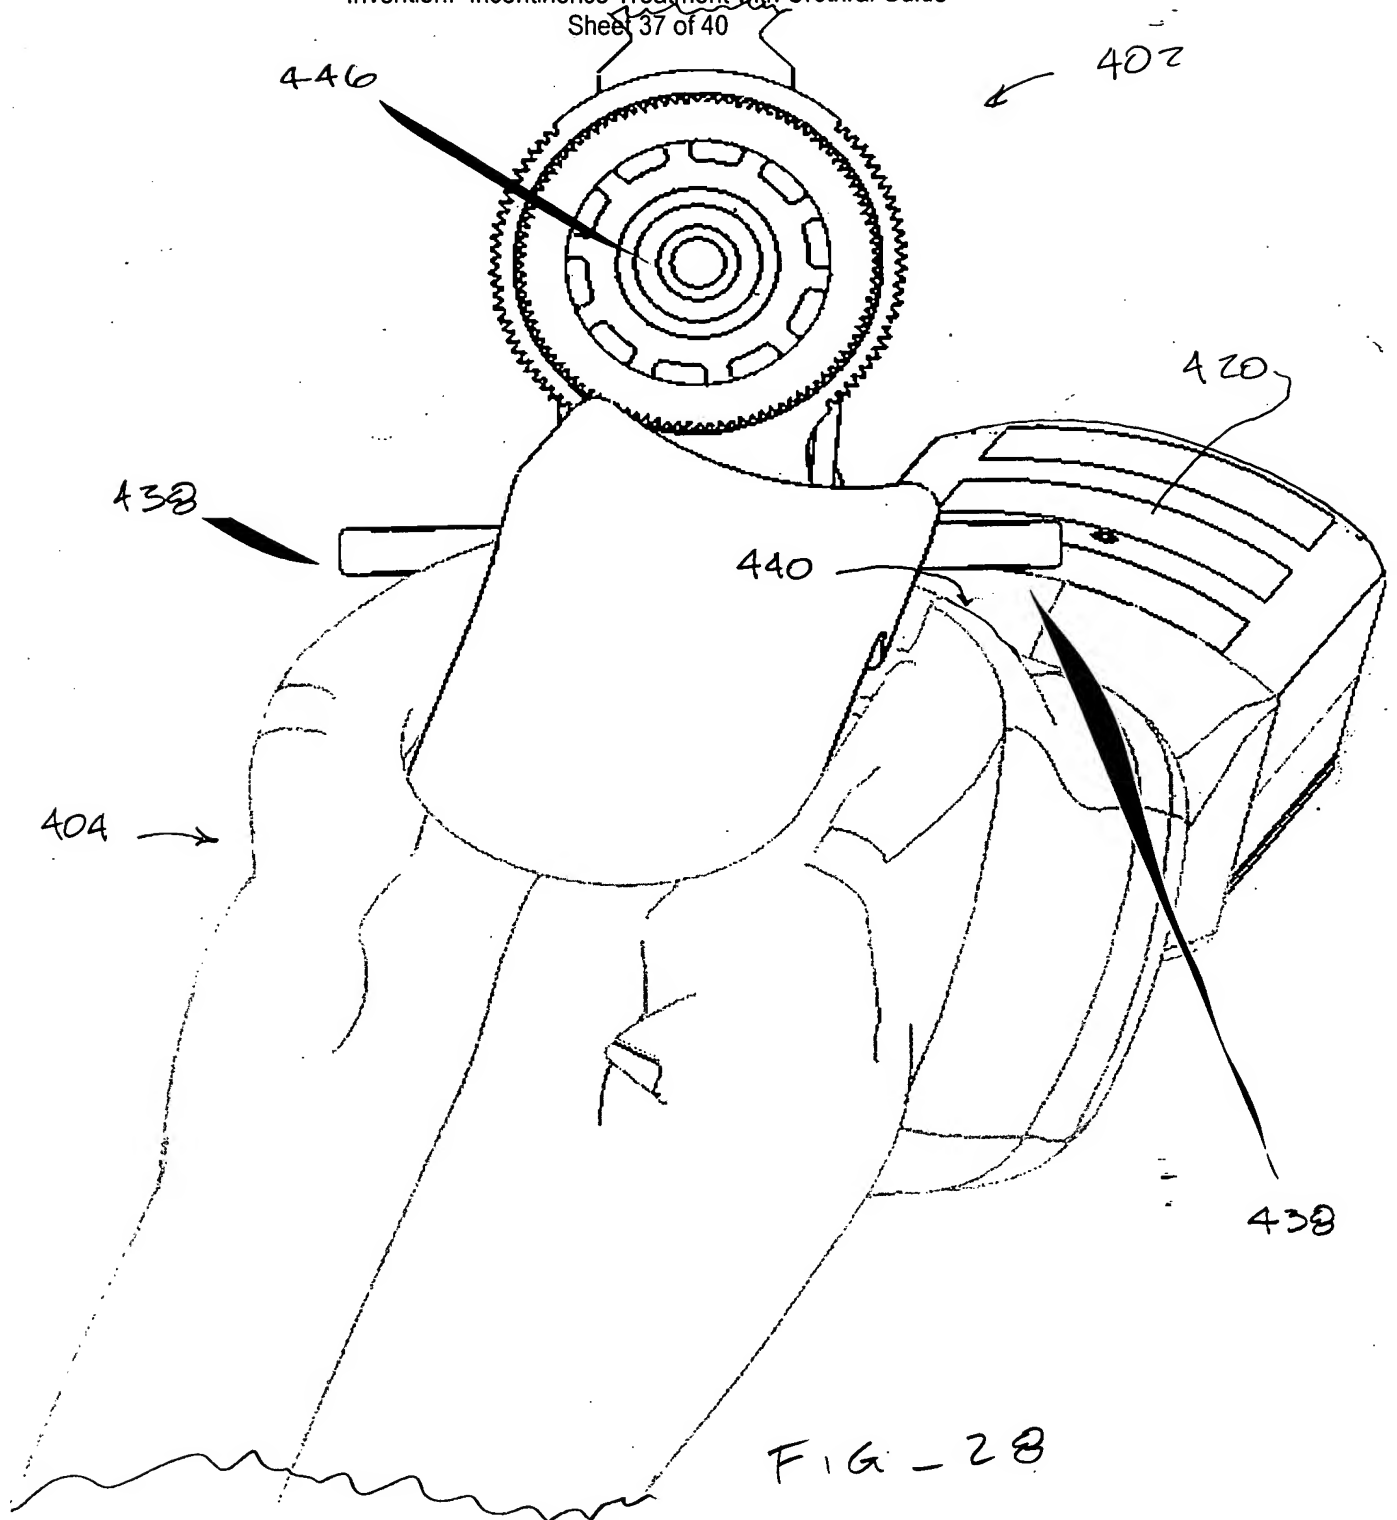


FIG - 27

BEST AVAILABLE COPY



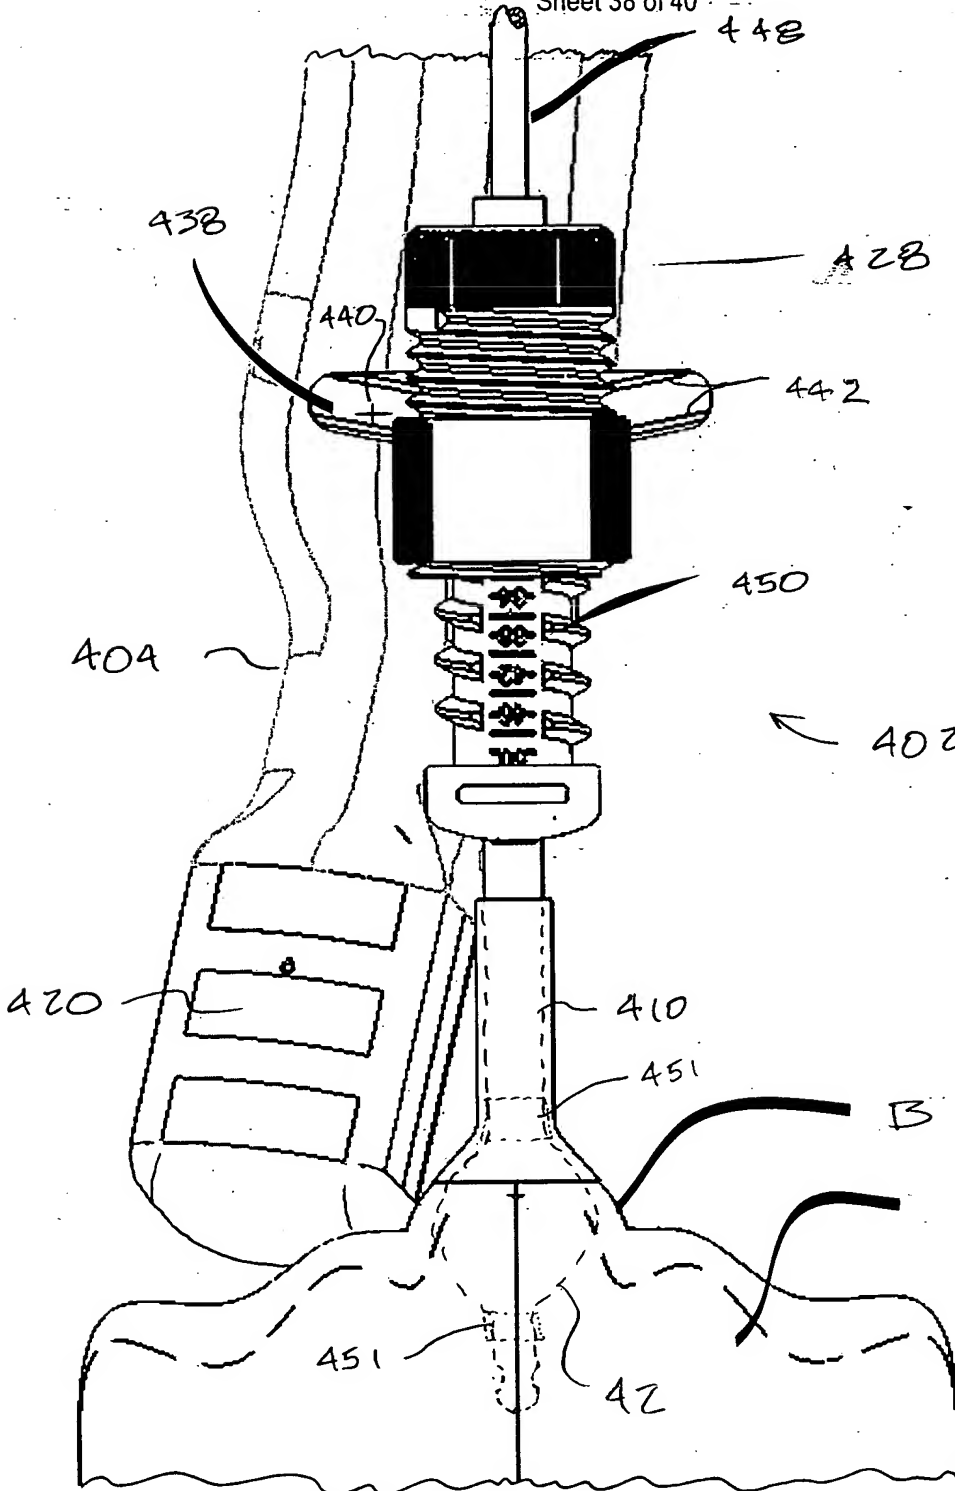


FIG. 29

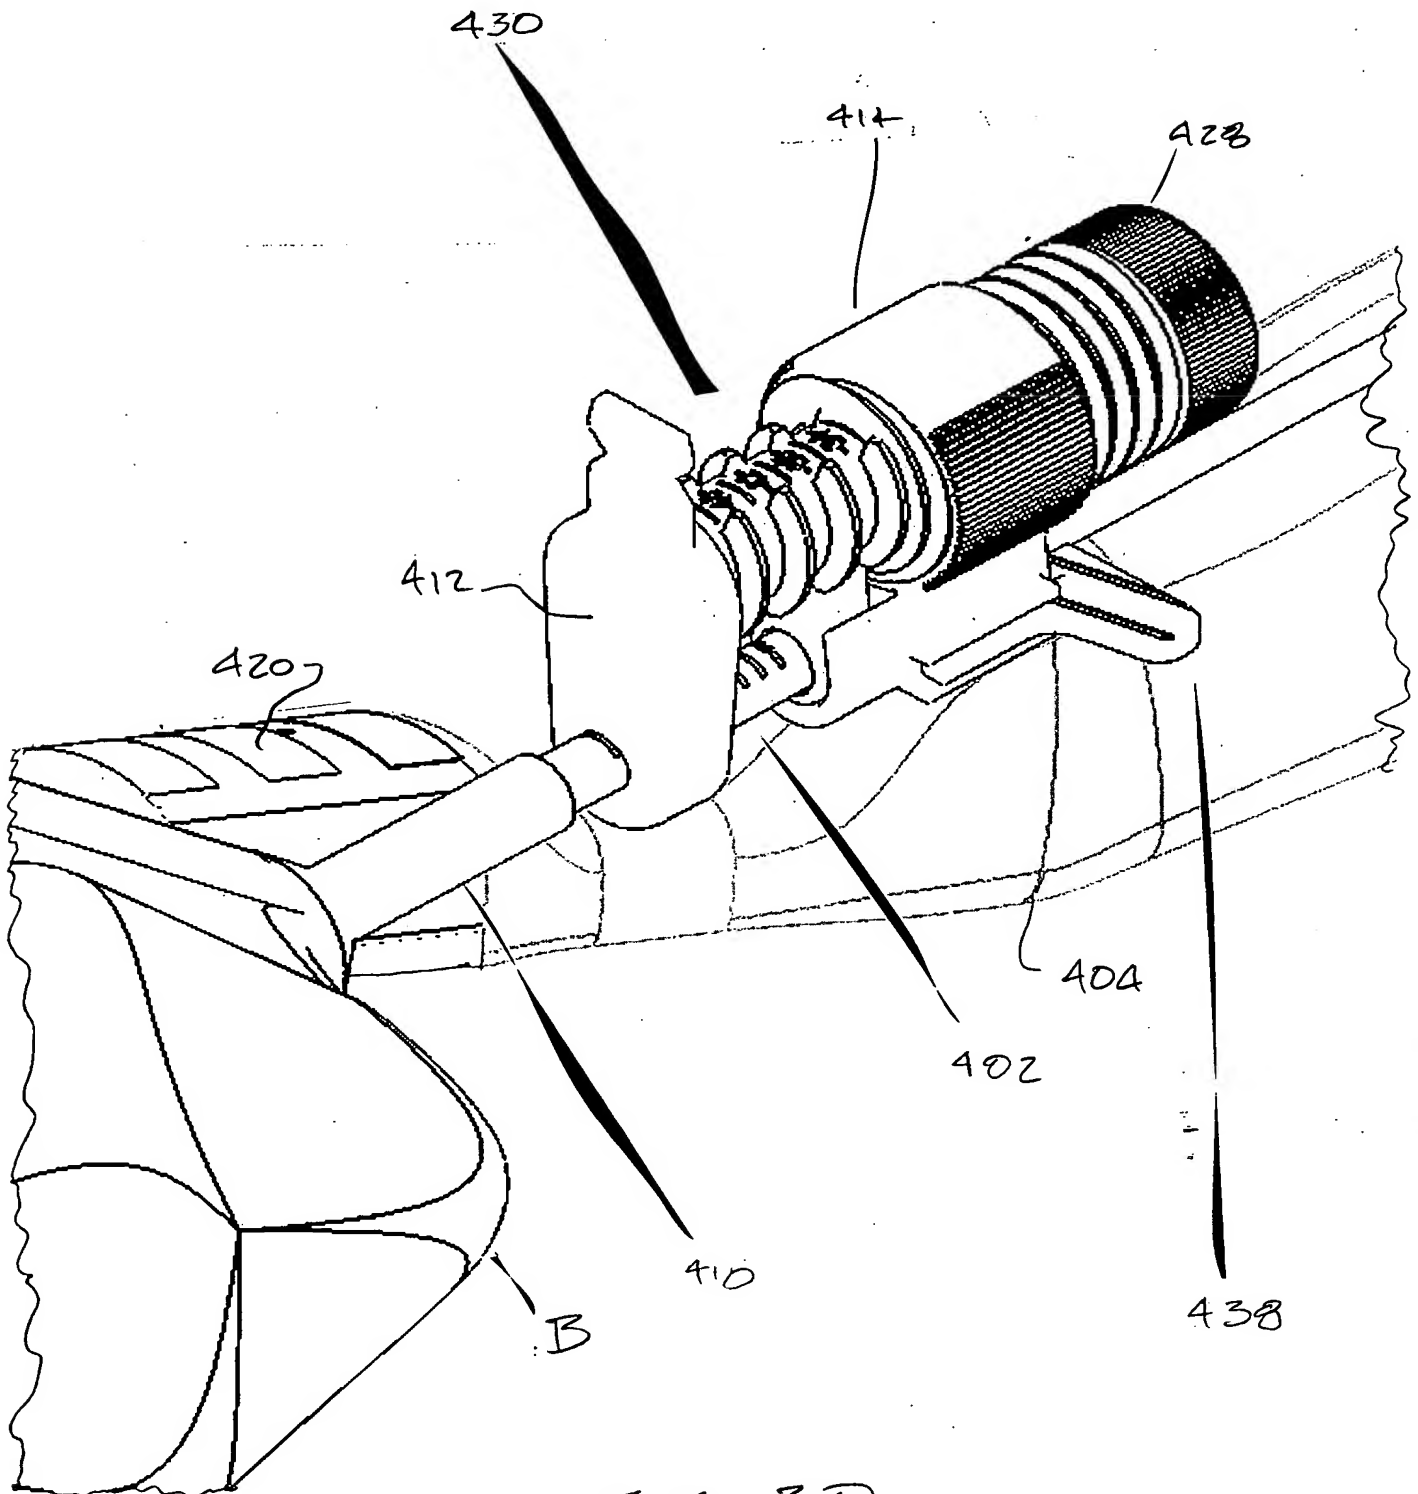


FIG. 30

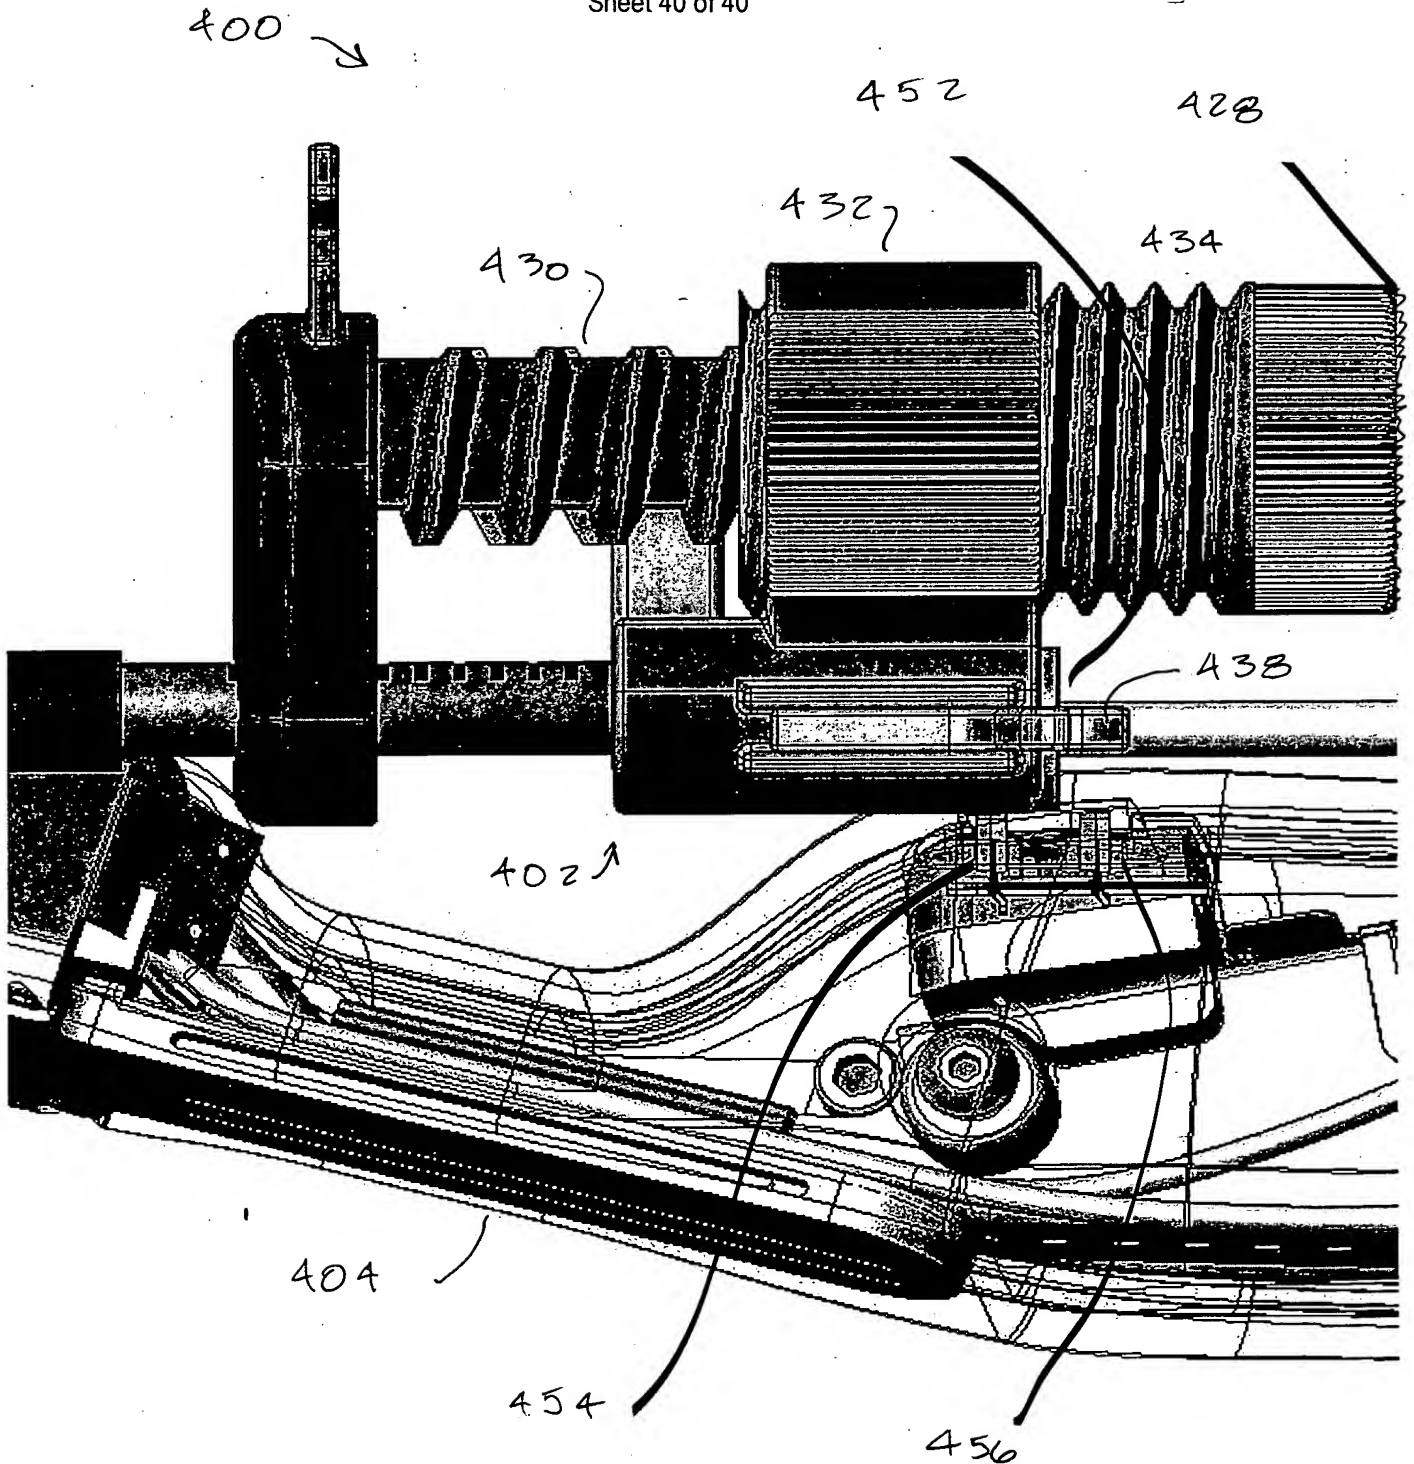


FIG - 31

BEST AVAILABLE COPY